

## TENOTAC<sup>®</sup> 2.0 SOFT TISSUE FIXATION SYSTEM

### Product Information

- Designed for reproducible less invasive correction of contracted toes and MPJ instability
- Cannulated implant designed to capture the flexor tendons, restoring balance to the toe
- Anatomic repair (fusion avoided) designed to maintain function proximally
- Designed for improved cosmesis with reduced swelling - no bony cuts or complicated soft tissue passes
- Patient specific correction allowing for the addition or removal of tension to position the toe in an ideal position

### Implant Features

#### Dorsal Sleeve




Small



Large




Low profile head to help prevent soft tissue irritation




Plantar tack and Dorsal sleeve implants are cannulated allowing for precise placement


#### Plantar Tack



Plantar Tack includes a washer to allow it to angulate up to 20 degrees



Single row of spikes allows for gripping of tendon



Holes allow for additional tendon hold

## Instrumentation




Ø0.9 mm K-wire




Ø1.1 mm K-wire



Dorsal Sleeve Driver



Dorsal Sleeve Standard Length Gauge

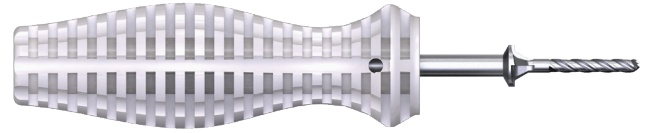


Ø2.8 mm Cannulated Drill/Standard Countersink with Handle



Plantar Tack Inserter

## Kit Configuration

### Sterile Packaged Kit

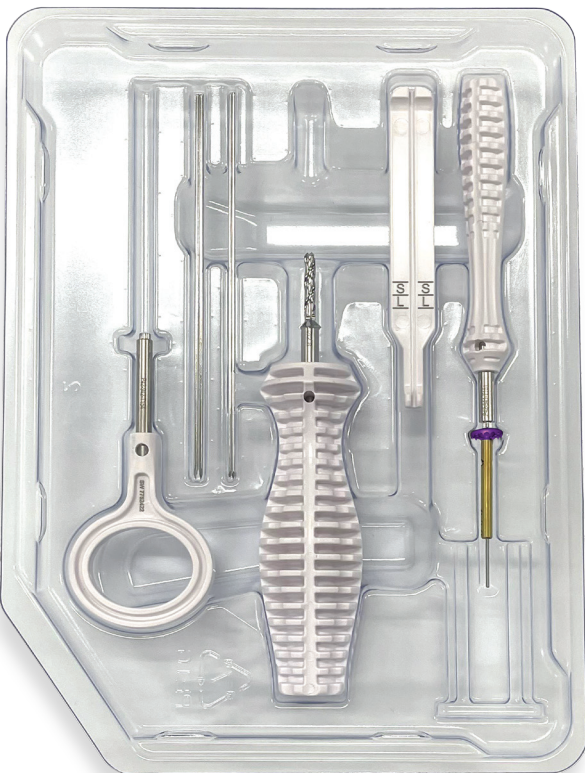

### TenoTac 2.0™ Soft Tissue Fixation System

Part Number	Description
P42-100-2265-SK	TenoTac 2.0™ Sterile Kit
P42-222-0075-S	Male Implant
P42-322-0065-S	Female Implant, Short
P42-322-0095-S	Female Implant, Long
P42-122-0125-S	TenoTac Female Implant, Extra Long (Hallux)
P42-822-0100-SK	TenoTac <sup>®</sup> Sterile Kit - Large (Hallux)



## Methods of Fixation

### TenoTac<sup>®</sup> Soft Tissue Fixation System Versatility:

The TenoTac Soft Tissue Fixation System is a unique offering due to its versatility and options for fixation. Depending on the specific digital deformity, the flexor digitorum brevis (FDB) or flexor digitorum longus (FDL) can be included or isolated to achieve desired correction. In addition, surgeons have the opportunity to increase or decrease tension applied to specific tendons to fine-tune correction if needed.



### Examples of use include:

- Replacement for Girdlestone-Taylor procedure for flexible hammertoes

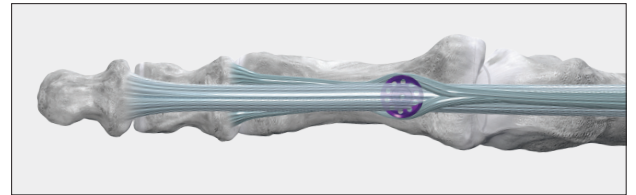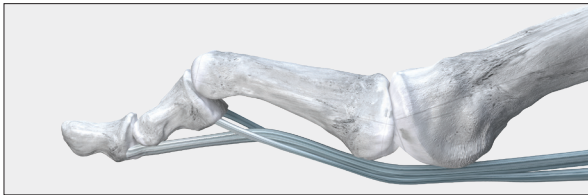



Tack FDB

- Used in conjunction with proximal interphalangeal joint (PIPJ) arthroplasty to stabilize the metatarsophalangeal joint

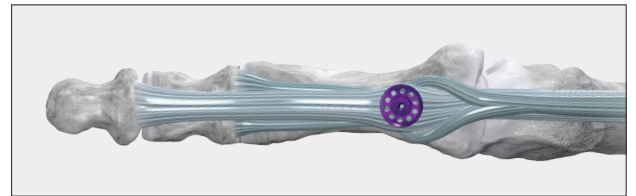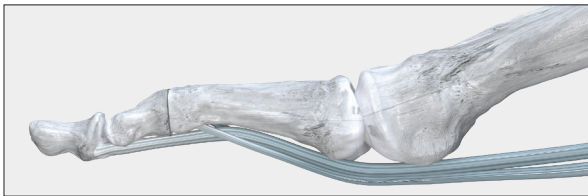


Tack FDB and FDL

- Used in conjunction with PIPJ arthrodesis to stabilize the metatarsophalangeal joint

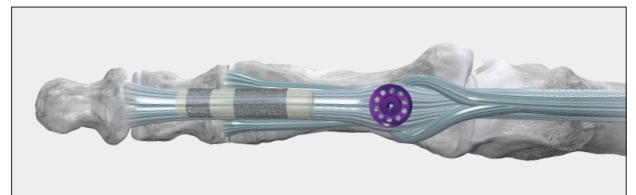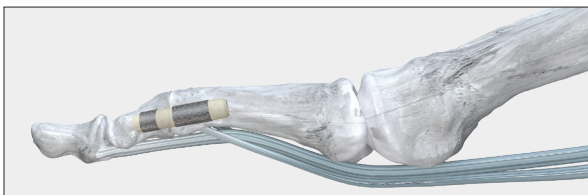

Tack FDB and FDL



- Combined with plantar plate repair to bolster the repair and correct the digital deformity

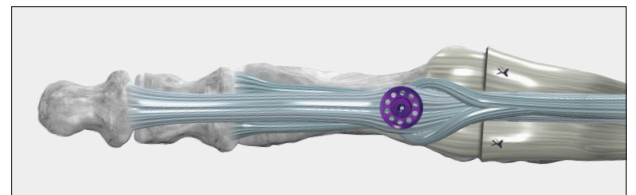

Tack FDB and FDL



## Methods of Fixation

- Used as a sole implant to correct flexible claw toe

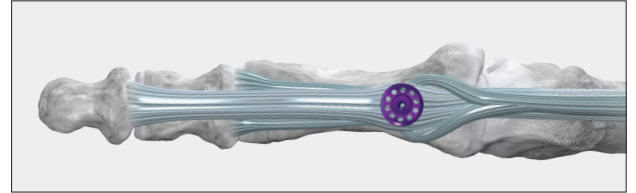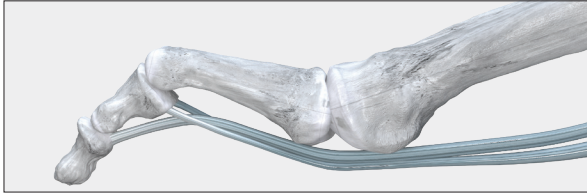

Tack FDB and FDL

- Used as a sole implant to correct flexible mallet toe

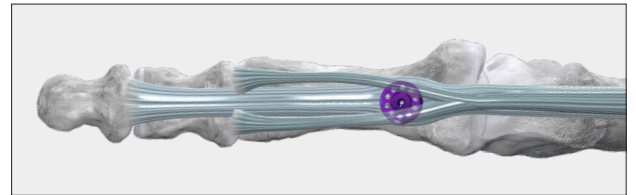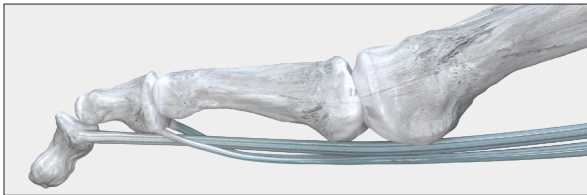

Tack FDL

## Teno Tac<sup>®</sup> Benefits

- Allows for controlled positioning and reapproximation of the toe - tension can be applied and backed off
- Avoids take down of the joint - reduced incision length, swelling, shortening, and potential for post-operative “sausage toe”
- Avoids complicated revisions associated with hammertoe implants (there are no bridges burned)
- Maintains function proximally - designed to allow patients to achieve push-off following the procedure

TTAC-01 RevD [2022-05-26]

™ Trademarks and ® Registered Trademarks of Paragon 28, Inc.  
 © Copyright 2022 Paragon 28, Inc. All rights reserved.  
 Patents: [www.paragon28.com/patents](http://www.paragon28.com/patents)

Paragon 28, Inc.  
 14445 Grasslands Dr.  
 Englewood, CO 80112 USA  
 (855) 786-2828

Paragon 28 Medical Devices Trading  
 Limited  
 First Floor Block 7 Beckett Way  
 Park West Business Park  
 Dublin 12  
 D12 X884  
 Ireland  
 +353 (0) 1588 0350

For the contraindications, potential complications and adverse reactions, warnings and precautions associated with this device, please refer to the device specific instructions for use at <http://www.paragon28.com/ifus>



For additional information on Paragon 28<sup>®</sup> and its products please visit [www.paragon28.com](http://www.paragon28.com)